

FORA®

ACTIVE WIRELESS plus P30 Plus BT



Quick Start User Guide

ForaCare Suisse AG
Neugasse 55, 9000 St. Gallen,
Switzerland
www.foracare.ch

MedNet EC-REP GmbH
Borkstraße 10, 48163 Münster,
Germany



REF FORA P30 plus BT




315-3129400-006

1 Single/Average Measurement




2




3


2~3cm /
0.8~1.2 inch

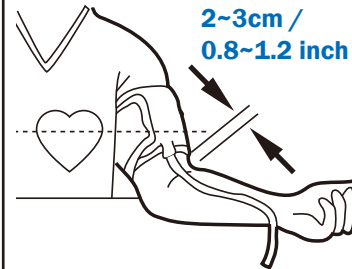


4

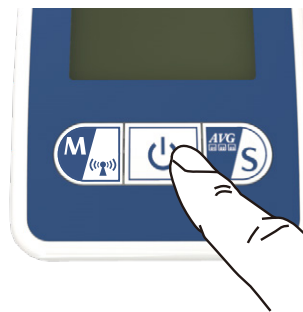


5

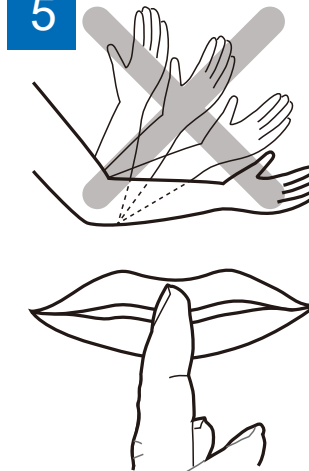



6

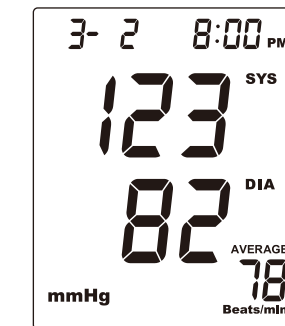

1 Auscultatory Mode

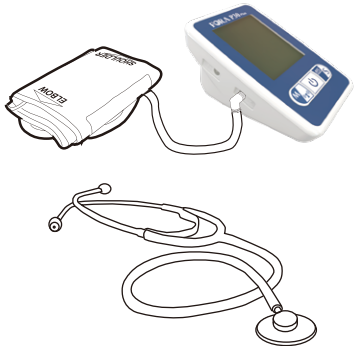


2

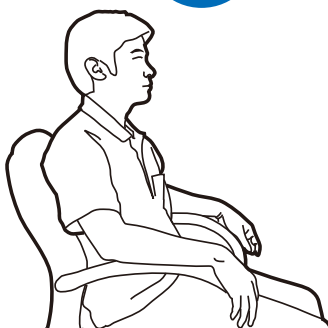

3

2~3cm /
0.8~1.2 inch

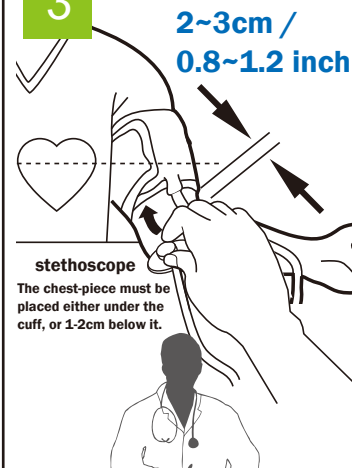

stethoscope


The chest-piece must be
placed either under the
cuff, or 1-2cm below it.

4



Press and hold until "AUS"
symbol appears on the display.


5

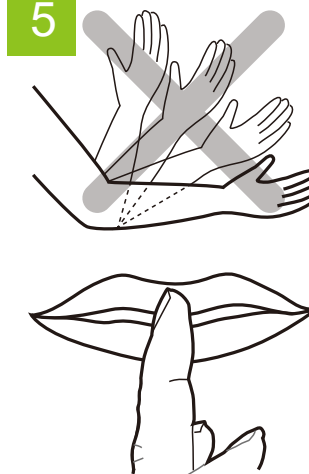



6





7

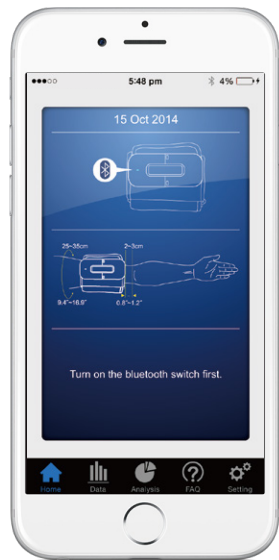



8

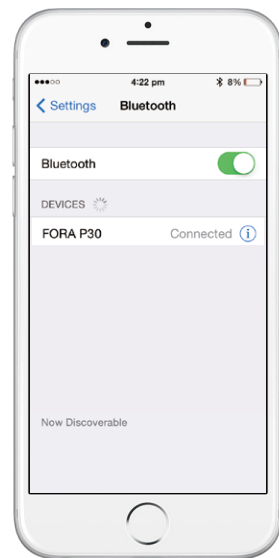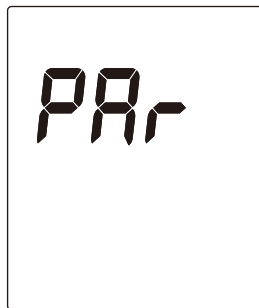

9

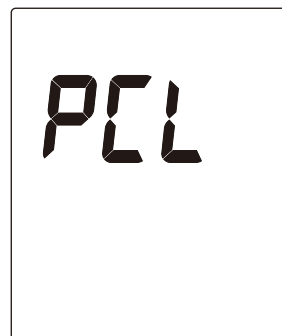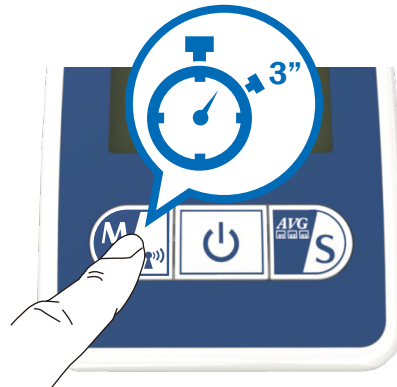

10

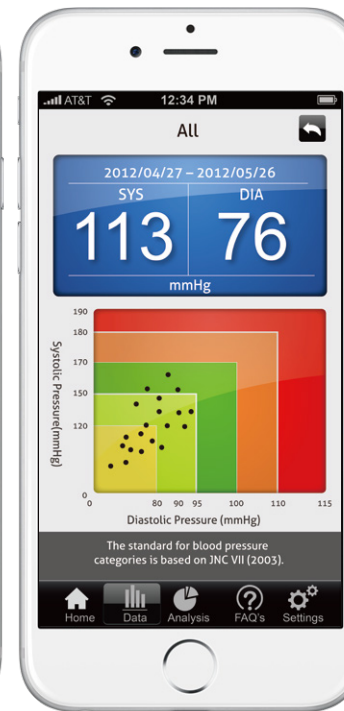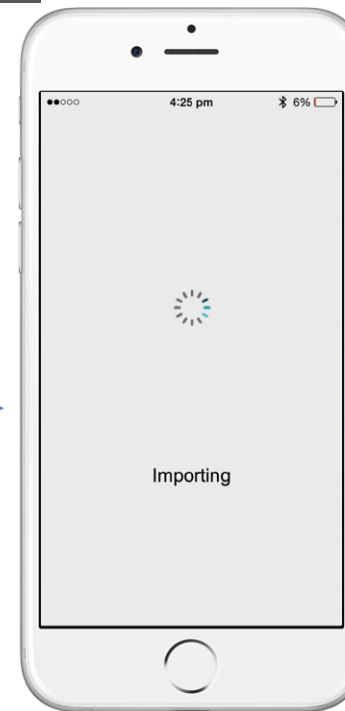

Apple and the Apple logo are trademarks of Apple Inc., registered in the U.S. and other countries. App Store is a service mark of Apple Inc.



Google Play and the Google Play logo are trademarks of Google LLC.

Q iFORA BP

