

Operating Instructions for All Metal Flow Switch

Model: SMN



1. Contents

1. Contents.....	2
2. Note	3
3. Instrument Inspection.....	3
4. Regulation Use	4
5. Operating Principle.....	4
6. Mechanical Connection.....	4
7. Electrical Connection	5
7.1. with Plug Connection.....	5
7.2. Example for Contact Protective Measures	5
8. Use in hazardous area	6
8.1. Statement an apparatus not containing an own potential ignition source	6
8.2. ATEX reed contact 41R57**	7
9. Maintenance and Care.....	14
10. Technical Information.....	14
11. Order Codes	16
12. Dimensions	16
13. Pressure Loss Diagram.....	17
14. EU Declaration of Conformance (SMN)	18
15. EU Declaration of Conformance (Reed contact 41R57**)... ..	19
16. Statement of conformity reed contact 41R57**	20

Manufactured and sold by:

Kobold Messring GmbH
Nordring 22-24
D-65719 Hofheim
Tel.: +49(0)6192-2990
Fax: +49(0)6192-23398
E-Mail: info.de@kobold.com
Internet: www.kobold.com



2. Note

Please read these operating instructions before unpacking and putting the unit into operation. Follow the instructions precisely as described herein.

The instruction manuals on our website www.kobold.com are always for currently manufactured version of our products. Due to technical changes, the instruction manuals available online may not always correspond to the product version you have purchased. If you need an instruction manual that corresponds to the purchased product version, you can request it from us free of charge by email (info.de@kobold.com) in PDF format, specifying the relevant invoice number and serial number. If you wish, the operating instructions can also be sent to you by post in paper form against an applicable postage fee.

The devices are only to be used, maintained and serviced by persons familiar with these operating instructions and in accordance with local regulations applying to Health & Safety and prevention of accidents.

When used in machines, the measuring unit should be used only when the machines fulfil the EC-machine guidelines.

as per PED 2014/68/EU

In acc. with Article 4 Paragraph (3), "Sound Engineering Practice", of the PED 2014/68/EU no CE mark.

Table 8, Pipe, Group 1 dangerous fluids

3. Instrument Inspection

Instruments are inspected before shipping and sent out in perfect condition. Should damage to a device be visible, we recommend a thorough inspection of the delivery packaging. In case of damage, please inform your parcel service / forwarding agent immediately, since they are responsible for damages during transit.

Scope of delivery:

The standard delivery includes:

- All Metal Flow Switch model: SMN



4. Regulation Use

Model SMN instruments monitor liquid flows. Only clean and homogeneous liquids of low viscosity - against which the instrument materials are resistant - should be monitored. Large switch-point inaccuracies can occur with highly viscous media.

Large dirt particles can block the float and thus cause faulty signals. Pieces of ferrite, deposited on the float (with embedded magnet) can lead to the same effect (we recommend magnetic filters).

5. Operating Principle

The KOBOLD model SMN flow switch is used when extremely low flow switch points are required in combination with minimum pressure loss at high flow rates.

The flow switch operates on the well-known float principle.

An orifice float with an integrated circular magnet moves within a cylindrical flow tube in the direction of the flow and against a spring.

The magnetic field of the float activates a reed contact which is mounted on the outside of the instrument in a sliding protective casing. Due to the special construction of the float and flow tube only a low flow is required to raise the float and hence to activate the reed contact. If the flow rate increases further and the float reaches the top of its travel an additional flow path opens allowing high flow rates without a significant increase in the pressure loss.

6. Mechanical Connection

- Make sure that allowed max. operating pressure and temperature are not exceeded.
- The instrument can be installed vertically or horizontally in the pipework. Flow is in the direction of the arrow from bottom to top, from left to right or from right to left.
- Remove all transport restraints and make sure that none of the packing material remains in the instrument.
- Use Teflon tape or something similar to seal the threaded connections.
- The instruments should not be installed in an induction field.
- If possible, check after mechanical installation that the threaded joint/pipe connection is tight and leakproof.




7. Electrical Connection


7.1. with Plug Connection

- Make sure that the electrical supply lines are powerless.
- Undo the locking screw on the plug cap and remove the cap from the base.
- Mount supply line in the plug cap as shown in the wiring diagram.
- The contact is adjusted and should not be modified.
- Insert the plug connector on the contact stem and fix it with the retaining screw.

N/O contact



Changeover contact




Attention! Every single specified electrical value for the sealed contact should not be exceeded even for short periods. We recommend contact protection relays or other contact protection measures for higher switching values.


When the external devices have been connected to the limit contact and the switching point has been set, the electrical connection is complete. The instrument can now be put into operation.

7.2. Example for Contact Protective Measures


For capacitive and inductive loads (long conductors and relay/protection) we recommend the following protective schemes.

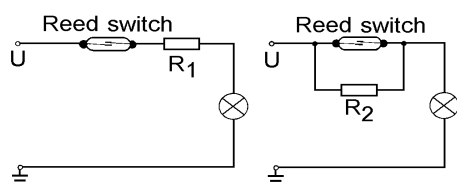


Lamp load with parallel or series resistance to the switch.

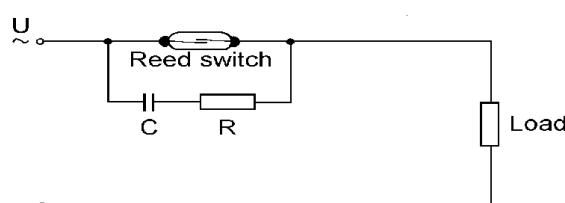

Protection with an RC circuit for a.c. current and inductive load.

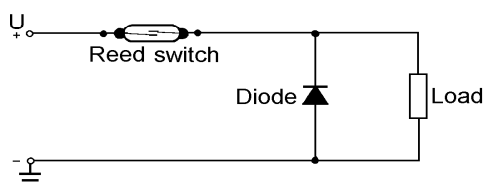

Protection with an idle diode for d.c. current and inductive load.

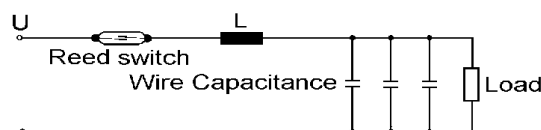

Protection against high discharge from condensers and load capacitances.



8. Use in hazardous area

8.1. Statement an apparatus not containing an own potential ignition source

Erklärung für Betriebsmittel ohne eigene potentielle Zündquelle in Anlehnung an die Richtlinie 2014/34/EU
TFR 17 HEK_BopZ 0013 Seite/page -1/ 2-

Statement an apparatus not containing an own potential source following Directive 2014/34/EU

Hiermit erklärt die / hereby declares

KOBOLD Messring GmbH, Nordring 22-24, DE 65719 Hofheim

in alleiniger Verantwortung, dass die Ergebnisse, der an den folgenden mechanischem Betriebsmitteln vorgenommenen Prüfungen, die Anforderungen der Richtlinie 2014/34/EU erfüllen.

that the results of the examinations with the mechanical equipment described below comply with the requirements of Directive 2014/34/EU.

Strömungswächter SMN, Identifikations-Nummer siehe Lieferunterlagen

Flowmeter/switch SMN, Identification number see shipping documents

sind gemäß Richtlinie 2014/34/EU, Artikel 1

are according to Directive 2014/34/EU, article 1

- a) keine Geräte,
- b) keine Schutzsysteme,
- c) keine Sicherheits-, Kontroll- oder Regeleinrichtungen,
- d) keine Komponenten.

- e) not an equipment,
- f) not a protective system
- g) not a safety device, controlling device or regulating device
- h) not a component.

Die mechanischen Betriebsmittel haben bei bestimmungsgemäßem Betrieb keine eigene potentielle Zündquelle und bekommen **keine Kennzeichnung** im Sinne der ATEX-Richtlinie. Eine interne Zündgefahrenbewertung wurde durchgeführt. Als Medium wird ein Fluid verwendet.

When used adequately, this mechanical equipment has no inherent potential ignition source and thus it is **not marked** in accordance with the ATEX- Directive. An internal ignition risk analysis was carried out. The used medium is a fluid.

Die mechanischen Betriebsmittel können, unter Berücksichtigung der geltenden Einrichtungsbestimmungen für Maschinen, Geräte und Anlagen im Ex-Bereich, z.B. EN 1127-1, EN 60079-14 u.a., folgendermaßen eingesetzt werden:

The apparatus can be used as follows in explosive atmospheres in accordance with the applicable erection regulations on machines, devices and plants, such as e.g. EN 1127-1, EN 60079-14, etc.:

- i) In der Zone 1 (Gas-Ex, Kategorie 2G) in den Explosionsgruppen IIA, IIB und IIC
- j) In der Zone 2 (Gas-Ex, Kategorie 3G) in den Explosionsgruppen IIA, IIB und IIC
- k) In der Zone 21 (Staub-Ex, Kategorie 2D) in den Explosionsgruppen IIIA und IIIB
- l) In der Zone 22 (Staub-Ex, Kategorie 3D) in den Explosionsgruppen IIIA und IIIB

- m) In Zone 1 (gas hazard, category 2G) in the explosion groups IIA, IIB and IIC
- n) In Zone 2 (gas hazard, category 3G) in the explosion groups IIA, IIB and IIC
- o) In Zone 21 (dust hazard, category 2D) in the explosion groups IIIA und IIIB
- p) In Zone 22 (dust hazard, category 3D) in the explosion groups IIIA und IIIB

Mögliche elektrische Betriebsmittel sind ohne Einfluss auf den mechanischen Zündschutz. Sie müssen den Anforderungen der jeweils vor Ort herrschenden Zonen genügen und sind nicht Bestandteil dieser Erklärung

Any electrical apparatus that may be used here do not impair the mechanical explosion protection. Those apparatus have to comply with the locally applicable zones and are not subject of this statement.

Folgende harmonisierte Normen/Spezifikationen sind in der am Unterschriftsdatum aktuellen Fassung angewandt worden:

The following harmonised standards and specifications were referred to in their version applicable on the date of signature:

⑩ EN 1127-1 Explosionsfähige Atmosphären, Explosionsschutz, Teil 1: Grundlagen und Methodik

⑩ EN 1127-1 Explosive atmospheres, Explosion prevention and protection, Part 1: Basic concepts and methodology

Wichtige Hinweise:

Please note:

- q) Die vom Hersteller erstellten Einbau und Bedienungsanleitungen sind zwingend zu beachten.
- r) Die im Anwenderland geltenden Errichtungsbestimmungen sind zu beachten.
- s) Die mechanischen Komponenten der SMV-Baureihe sind für Umgebungstemperaturen: -10 °C .. 90 °C
- t) Bei bestimmungsgemäßem Betrieb wird außen eine Erwärmung < 10 K erwartet; die Temperaturklasse T4 wird eingehalten.
- u) Sämtliche außen liegenden Werkstoffe bestehen aus geeigneten funkenarmen Materialien, kein Leichtmetall. Der Betreiber ist

- cc) The installation and operating instructions provided by the manufacturer are to be considered compellingly.
- dd) The installation regulations valid in the designated country of use are to be observed.
- ee) The SMN series with its mechanical components is suitable for ambient temperatures of -10 °C .. 90 °C
- ff) At intended operation the temperature rising outside is < 10 K; Temperature class T4 is kept.
- gg) All exterior materials consist of suitable low-sparking components no alloy. The operator himself, however, is responsi-



Erklärung für Betriebsmittel ohne eigene potentielle Zündquelle in Anlehnung an die Richtlinie 2014/34/EU

TFR 17 HEK_BopZ 0013

Seite/page -2/ 2-

Statement an apparatus not containing an own potential source following Directive 2014/34/EU


jedoch für die Überprüfung der Zündgefahr durch Funken beim Betrieb der kompletten Maschine selbst verantwortlich.

- v) Die mechanischen Komponenten des SMN müssen in den Potentialausgleich einbezogen werden.
- w) Anschlussleitungen von elektrischen Betriebsmitteln sind geschützt zu verlegen.
- x) Wenn isolierende Anschlussrohre verwendet werden, dann sind Typen mit einem Durchmesser < 20 mm (IIC) oder < 30 mm (IIA, IIB, Staub) zulässig.
- y) Staubablagerungen sind regelmäßig zu entfernen.
- z) Bei Undichtigkeit des Gehäuses darf das Betriebsmittel nicht weiter betrieben werden
- aa) Streuströme (z.B. in Anlagen mit elektrischem Korrosionsschutz) dürfen nicht über die Bauteile geführt werden
- bb) Bei Montagen im Ex-Bereich ist unbedingt die EN 1127-1 Anhang A zu beachten (ggf. funkenarmes Werkzeug benutzen!)

Ausgefertigt in Hofheim am 3. Juni 2019

Unterzeichnet für und im Namen der Kobold GmbH

Ort und Datum

Manfred Wenzel  Prokurist / authorized signatory

ble for checking the risk of ignition caused by sparks during the operation of the complete machine.

- hh) The mechanical components of the SMN have to be integrated in the equipotential bonding.
- ii) Connecting cables of electrical apparatus have to be installed in a protected manner.
- jj) If insulated connection pipes are used, only types with a diameter < 20 mm (IIC) or < 30 mm (IIA, IIB, Dust) may be used.
- kk) Dust deposits are to be removed regularly.
- ll) If the enclosure shows signs of leakage, the apparatus may be not operated further.
- mm) Leakage currents (e.g. in plants with electrical anti-corrosion protection) may not be led over the parts.
- nn) When mounting the apparatus inside an explosive area, Annex A of standard EN 1127-1 has to be adhered to (if necessary, low-sparking tools have to be used).

Issued at Hofheim on June 3rd, 2019

Signed for and on behalf of Kobold GmbH

HEK_BopZ 17 xxxx Ergänzung 1 Kobold SMV/odt

8.2. ATEX reed contact 41R57**

ATEX N/O contact 41R57

-  II 3G Ex ic IIC T4 Gc
-  II 3 D Ex ic IIIC T125 °C Dc
- 20 °C ≤ Ta ≤ 80 °C
- max. 250 V_{AC/DC}/1.5 A/100 W/100 VA

ATEX changeover contact 41R57U

-  II 3G Ex ic IIC T4 Gc
-  II 3 D Ex ic IIIC T125 °C Dc
- 20 °C ≤ Ta ≤ 80 °C
- max. 250 V_{AC/DC}/1 A/30 W/60 VA

Ex-relevant excerpt of the operating instructions of the reed contact 41R57 **

1. Preamble

This excerpt of the operating instructions only represents the ex-relevant aspects. It is copied into the original operating manual in the same or analogous form; Textual changes are permitted, the ex-relevant statements remain.

To ensure the function and for your own safety, please read the enclosed operating instructions carefully before you begin the installation. If you have any questions, please contact the KOBOLD Messring GmbH, Hofheim. It applies with the original operating instructions.

The following standard issues were considered in the evaluation of the product:

- a) IEC 60079-0:2017 Ed. 7 / EN 60079-0:2018 Explosive atmospheres – Part 0: Equipment - General requirements
- b) IEC 60079-11:2011 Ed. 6 + Corr. 2012 / EN 60079-11:2012 Explosive atmospheres - Part 11: Equipment protection by intrinsic safety "i"

2. General information on explosion protection

The reed switches work together with various KOBOLD products and serve there for monitoring. It is available as N/O contact or changeover contact.

The electrical connection is made via a plug - only in intrinsically safe systems.

The reed switch is intended for commercial use and may only be used in accordance with the specifications in the technical documentation of Kobold and the information on the nameplate. It is only operated together with certified products via an intrinsically safe circuit. They comply with the valid standards and regulations.

The installation regulations (e.g. EN 60079-14) for systems in potentially explosive atmospheres must be observed.

Further important details can be found in the corresponding EC-type examination certificate.

Permitted use

- The intrinsically safe reed switch can be used as follows:
 - In Zone 2 (Gas-Ex, EPL Gc) in explosion groups IIA, IIB and IIC
 - In Zone 22 (Dust-Ex, EPL Dc) in explosion groups IIIA, IIIB and IIIC
- The requirements for simple electrical equipment for use in intrinsically safe circuits in zones 1/21 are fulfilled.
- The qualification regarding the surface temperature is T4. For all gases, vapors, mists with an ignition temperature > 135 ° C the equipment is not an ignition source.
 - In the dust Ex area, 125 ° C is the reference temperature for further consideration regarding the safety distance from the smoldering temperature.
- The ambient temperature range is -20 ° C ≤ Ta ≤ 80 ° C.



2.1. Electrical characteristics for Ex i

Electrical data:

- Rated voltage up to 45 volt AC / DC
- Rated current up to 2 A
- $U_{iIC} \leq 30 \text{ V AC / DC}$, $I_{iIC} \leq 250 \text{ mA}$
- $U_{iIB} \leq 45 \text{ V AC / DC}$, $I_{iIB} \leq 2 \text{ A}$
- $U_{iIIC} \leq 45 \text{ V AC / DC}$, $I_{iIIC} \leq 250 \text{ mA}$
- $L_i = \text{negligible}$, $C_i = \text{negligible}$
- Heating on the outer housing $< 15 \text{ K}$

2.2 Type code

The equipment is identified by the following type code:

Type	Description	Item-No.	Remarks
41R57 A B	Type coding		
41R57	Contact device		
A	N/O contact (2 wires), Plug with black cap		
	Change-over contact (3 wires), Plug with grey cap		
B	70 – 75 with marking (not ex-relevant)	202.289	N/O
	45 – 50 with marking	202.285	N/O
	50 – 55 with marking	202.286	N/O
	60 – 65 with marking	202.287	N/O
	70 – 75 with marking	202.288	Change-over
	60 – 65 change-over contact	202.290	Change-over

2.3 Temperature class

The reed switch is suitable for temperature class T4 / T125 ° C.

2.4 General requirements

2.4.1 Intended Use

- To ensure safe operation, the products may only be used according to the instructions in the assembly instructions. During use, the legal and safety regulations required for the respective application must be observed in addition. This applies analogously when using accessories.
- Failure to comply with the instructions given in this excerpt or in the case of improper handling of the product will render our liability null and void. In addition, the warranty on products and spare parts is void.
- The products are not safety elements in terms of their intended use.
- Only original parts of the manufacturer may be used.



2.4.2 General safety instructions

The reed switch corresponds to the state of the art and is reliable. The reed switch may pose a residual hazard if improperly used and operated by untrained personnel.

Every person, responsible for the installation, commissioning, maintenance or repair of the reed switch, must have read and understood the assembly instructions and in particular the safety instructions.

- a) Follow the general rules of technology for the selection and proper operation of a product.
- b) All connected electrical and mechanical equipment must be suitable for the respective application.
- c) Observe the notes in these operating instructions as well as the conditions of use and permissible data that appear from the imprints / nameplates of the respective products.
- d) It must be ensured that only product protection types corresponding to the zones are installed!
- e) The product is only approved for proper and intended use in a normal industrial atmosphere. Immersion in liquids is not permitted.
- f) It must be ensured that no falling objects can hit the product.
- g) The operator must ensure the lightning protection for the entire system in accordance with local regulations.
- h) It is the responsibility of the installer to ensure that the function of the reed switch in conjunction with the individual evaluation devices functions properly and is approved for the intended use.
- i) The intrinsically safe connection - including the reed switches - must be made via approved / tested evaluation devices, which may need to be equipped with suitable zener barriers or switching amplifiers.

3. Commissioning, installation

Depending on the IP degree of protection, the time for cleaning the equipment (dust deposits) must be specified. Other important facts:

- a) The product may be put into operation in Zone 2 (Cat. 3G, EPL Gc) or in Zone 22 (Cat. 3D, EPL Dc) in intrinsically safe circuits only by specialists with a qualification similar to a qualified person according to TRBS 1203.
- b) The requirements for simple electrical equipment that apply to the hazardous area of Zones 1/21 according to EN 60079-11 are fulfilled.
- c) The products may only be used in the usual industrial atmosphere. In the presence of aggressive substances in the air, the manufacturer must always be consulted. The products must be adequately protected in adverse environmental conditions.
- d) Operation of the product is only permitted in fully assembled and undamaged enclosures. In case of possible damage, a zone carryover may have to be considered by the operator; Moreover, operation of the housing is not permitted if the housing is damaged.
- e) The environmental conditions specified in the operating instructions must be adhered to and protected against adverse environmental conditions.



- f) Heat radiation from foreign products / components must also be considered.
- g) The reed switch must be protected against inadmissible access of liquids and / or soiling.
- h) Fixed parts (e.g. due to frost or corrosion) must not be loosened by force in the presence of an explosive atmosphere. Icing must therefore be avoided.
- i) The reed switch may only be subjected to minor vibrations, see also IEC 34-14.
- j) To ensure the discharge of electrostatic charges, the national requirements must be considered.
- k) In particular, isolated capacities must be prevented.
- l) Only those zener barriers or switching amplifiers may be used whose output circuits are approved / tested for use in potentially explosive atmospheres. In Europe, use in Zones 1/21 requires an EC type-examination certificate for the equipment concerned issued by a body designated for explosion protection.
- m) The voltage of the supply units must be less than or equal to the voltage U_i of the reed switch.
- n) The total current I_o of the supply units must be less than or equal to the current I_i of the reed switch.
- o) For the installation of the intrinsically safe circuit, a control drawing (system description) to be created by the installer / operator is required.
- p) Equipotential bonding must be established along the intrinsically safe circuit when using a grounded supply.
- q) The certificates must be taken into account, including the special conditions specified therein.
- r) Resistant parts of the product (e.g. due to frost or corrosion) must not be forcibly loosened in the presence of an explosive atmosphere.
- s) Within the potentially explosive area, installation may only be carried out taking into account the locally applicable installation regulations. The following conditions must be observed (incomplete):
- t) Installation and maintenance may only be carried out in an explosion-free atmosphere and in compliance with the regulations in force in the country of the operator.
- u) Additional precautions must be taken if the presence of hydrogen sulphide, ethylene oxide and / or carbon monoxide is to be expected: these substances have very low ignition energy!
- v) In the presence of these substances and in the presence of a substance of the explosion group IIC and in the case of presumably existing potentially explosive atmosphere, only spark-free tools may be used!



4. Maintenance, servicing

Definition of terms according to IEC 60079-17:

Maintenance and Repair: A combination of all activities performed to maintain or recover an item in a condition that meets the requirements of the specification in question and ensures the performance of the required functions.

Inspection: An activity involving the careful examination of an object, with the aim of obtaining a reliable statement of the condition of the object, carried out without disassembly or, if necessary, with partial disassembly, supplemented by measures such as measurements becomes.

Visual inspection: A visual inspection is a test that detects visible faults, such as missing screws, without the use of access devices or tools.

Close-up Test: A test that identifies, in addition to the aspects of visual inspection, such errors, such as loose screws, which can only be obtained by using access devices, such as a screwdriver, e.g. steps (if necessary), and tools are visible. For close-up tests, housing usually does not need to be opened or the equipment must be de-energized.

Detail test: A test that detects, in addition to the aspects of close-up testing, such defects as, for example, loose connections that can only be recognized by opening housings and / or, if necessary, using tools and test equipment.

- a) Maintenance measures may only be carried out by qualified persons.
- b) Only use accessories in potentially explosive atmospheres that comply with all requirements of European directives and national legislation.
- c) Maintenance measures with dismantling of the reed switch may only be carried out in an ex-free atmosphere.
- d) The replacement of components may only be carried out with original spare parts, which are also approved for use in potentially explosive areas.
- e) The products must be regularly maintained and cleaned in the Ex area. The intervals are set by the operator according to the environmental demands on site.



	Activity	visual inspection per month	Close inspection every 6 months	detailed inspection every 12 months
1	Visual inspection of the reed switch for damage, remove dust deposits	•		
2	Check for integrity and function			•
3	Testing the entire system	The responsibility of the operator		


5. Troubleshooting

Products operated in conjunction with potentially explosive atmospheres must not be modified. Repairs to the product may only be performed by specially trained and authorized personnel.

6. Disposal

Disposal of the packaging and used parts must be in accordance with the regulations of the country in which the product is installed.

7. Marking of the reed switch (nameplate)

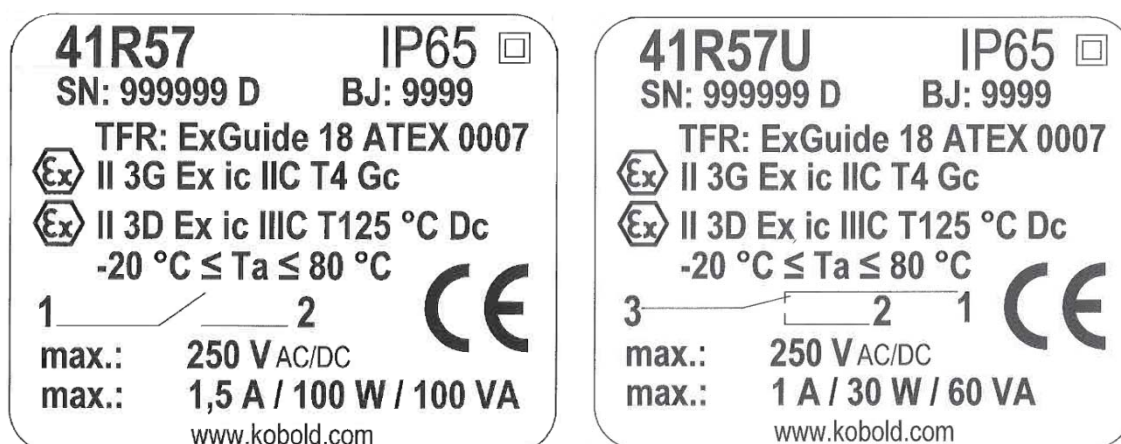

In the serial number the year of manufacture can be coded; optionally, it can also be specified as plain text.

As a rule, a readable marking has been made for the type of explosion protection required in field use - even before the product is put into operation for the first time.

A reed switch that has already been operated in non-intrinsically safe circuits may no longer be used in intrinsically safe circuits later on.

9. Maintenance and Care

The instrument needs no maintenance when the measured medium is not polluted. Lime and other deposits should be removed regularly from the inside parts of the instruments. The instrument **cannot** be taken apart and must be cleaned with a suitable cleanser.

10. Technical Information

Housing:	SMN-11...: brass, Ms 58 SMN-12...: stainless steel, 1.4301
Float:	SMN-11...: brass, Ms 58 SMN-12...: stainless steel, 1.4301
Cage:	SMN-11...: brass, Ms 58 SMN-12...: stainless steel, 1.4301
Spring:	stainless steel
Magnets:	Ceramic
Max. temperature:	100 °C
Max. pressure:	SMN-11...: 250 bar SMN-12...: 350 bar
Installation position:	horizontal or vertical (upward direction), flow in direction of the arrow
Contact components:	1 bistable reed contact N/O contact, changeover contact,
Electrical connection:	Connector DIN 175301-803
Electrical switching values:	N/O contact (standard) max. 250 V _{AC/DC} / 1,5 A / 100 W / 100 VA changeover contact (Standard) max. 250 V _{AC/DC} / 1 A / 30 W / 60 VA N/O contact and changeover contact (cCSAus) max. 230 V _{DC} / 0,26 A / 60 W, 60 V _{DC} / 1 A / 60 W max. 240 V _{AC} / 0,42 A / 100 W, 100 V _{AC} / 1 A / 100 W
Accuracy:	± 5% f. s.



Use in hazardous areas

Mechanics:

The apparatus can be used as follows in explosive atmospheres in accordance with the applicable erection regulations on machines, devices and plants, such as e.g. EN 1127-1, EN 60079-14 etc.:

- a) In Zone 1 (gas hazard, category IIG) in the explosion groups IIA, IIB and IIC
- b) In Zone 2 (gas hazard, category IIIG) in the explosion groups IIA, IIB and IIC
- c) In Zone 21 (dust hazard, category IID) in the explosion groups IIIA and IIIB
- d) In Zone 22 (dust hazard, category IIID) in the explosion groups IIIA and IIIB

ATEX N/O contact 41R57

...G0 and GG:

 II 3 G Ex ic IIC T4 Gc
 II 3 D Ex ic IIIC T125 °C Dc
 $-20\text{ °C} \leq T_a \leq 80\text{ °C}$
 max. 250 V_{AC/DC}/1.5 A/100 W/100 VA

ATEX changeover contact 41R57U

...H0 and HH:

 II 3 G Ex ic IIC T4 Gc
 II 3 D Ex ic IIIC T125 °C Dc
 $-20\text{ °C} \leq T_a \leq 80\text{ °C}$
 max. 250 V_{AC/DC}/1 A/30 W/60 VA

Hysteresis:

approx. 3.5 mm float movement

Protection:

IP 65 (electr. contact)

IP 54 (side indicator)




11. Order Codes


Order Details (Example: SMN-1150H R0 R 25)

Function	Brass version	Stainless steel version	Type of contact	Connection
Max Flow: 100 l/min Fix Switch point at approx. 1l/min with falling flow rate	SMN-1150 H...	SMN-1250 H...	..R0.. = 1 N/O contact ..U0.. = 1 changeover contact ..C0.. = 1 N/O contact (cCSAus) ..D0.. = 1 changeover contact (cCSAus) ...G0... = 1 ATEX N/O contact (model 41R57) ...H0... = 1 ATEX changeover c. (model 41R57U)	...R25 = G1 female ...N25 = 1 NPT female

12. Dimensions

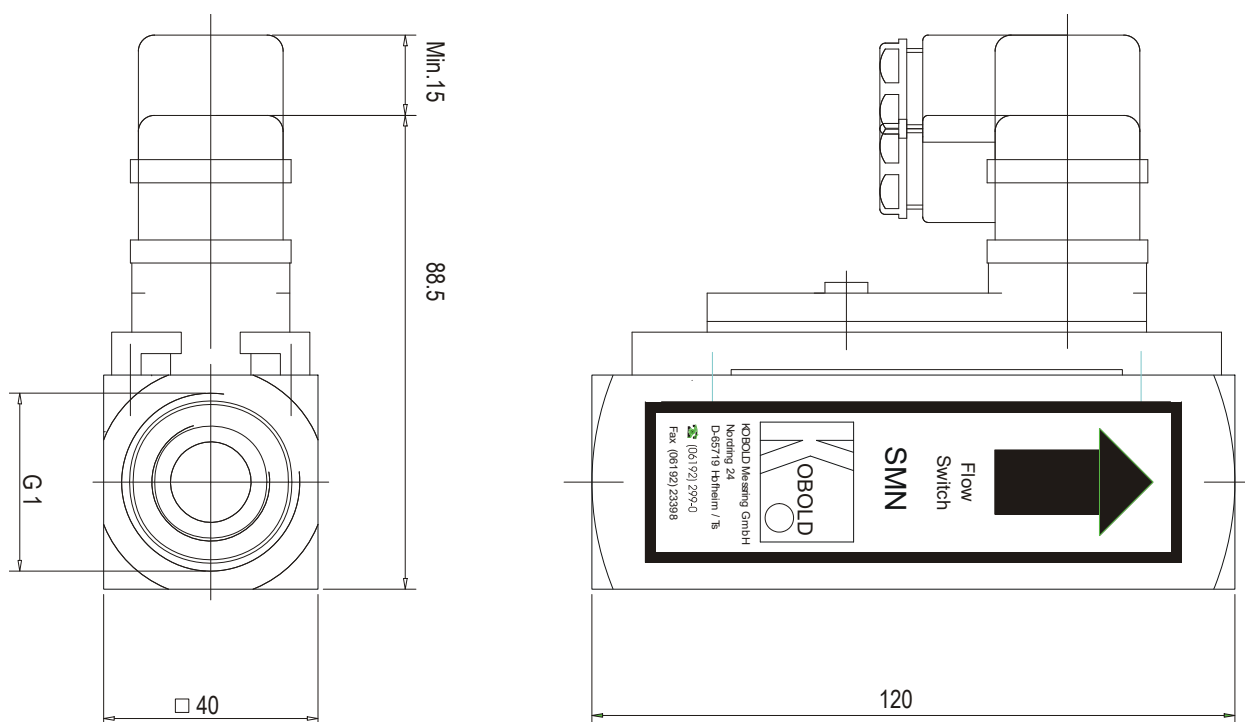

13. Pressure Loss Diagram

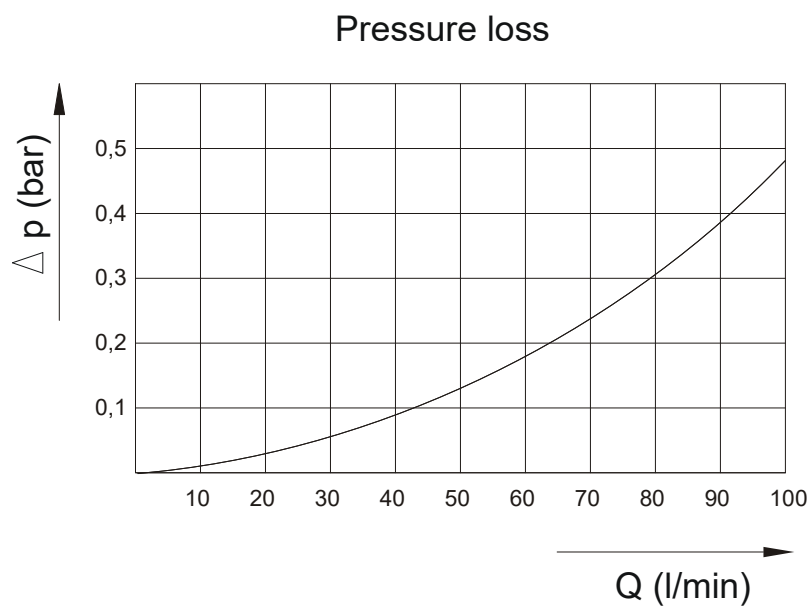

14. EU Declaration of Conformance (SMN)

We, KOBOLD-Messring GmbH, Hofheim-Ts, Germany, declare under our sole responsibility that the product:

All Metal Flow Switch

model: SMN-...

to which this declaration relates is in conformity with the standards noted below:

EN 61010-1:2011

Safety requirements for electrical equipment for measurement, control and laboratory use - Part 1: General requirements

EN 60529:2014

Protection type through case (IP code)

EN IEC 63000:2018

Technical documentation for the assessment of electrical and electronic products with respect to the restriction of hazardous substances

Also, the following EC guideline is fulfilled:

2014/35/EU

Low Voltage Directive

2011/65/EU

RoHS (category 9)

2015/863/EU

Delegated Directive (RoHS III)

Hofheim, 28 April 2022



H. Volz
General Manager



M. Wenzel
Proxy Holder



15. EU Declaration of Conformance (Reed contact 41R57**)

EU-KONFORMITÄTSERKLÄRUNG zur Bestätigung der
Übereinstimmung einer Baugruppe mit der Richtlinie
2014/34/EU

EU DECLARATION OF CONFORMITY to confirm
the conformance of a device with the Directive
2014/34/EU

Der Hersteller

The manufacturer

KOBOLD Messring GmbH, Nordring 22-24, DE 65719 Hofheim

erklärt hiermit in alleiniger Verantwortung, dass die nachfol-
gende Maschine oder Baugruppe

hereby declares under sole responsibility, that the
machinery or subassembly equipment described be-
low

Bezeichnung

Description

Reed-Schalter / Reed contact 41R57**

Kennzeichnung / Marking:  II 3G Ex ic IIC T4 Gc or  II 3D Ex ic IIIC T125 °C Dc

Fertigungs-Nummer lt. Lieferpapieren und Typenschild

Serial number see shipping documents and type la-
bel

mit den Bestimmungen folgender harmonisierter Normen der
Europäischen Union:

conforms with the provisions of the following harmo-
nized standards in the version of the European
Union:

- IEC 60079-0:2017 Explosionsgefährdete Bereiche –
Teil 0: Betriebsmittel - Allgemeine Anforderungen
- EN 60079-11:2012 Explosionsgefährdete Bereiche – Teil
11: Geräteschutz durch Eigensicherheit "i"

- IEC 60079-0:2017 Explosive atmospheres –
Part 0: General Requirements
- EN 60079-11:2012 Explosive atmospheres – Part
11: Equipment protection by intrinsic safety "i"

Ebenfalls mit folgenden Europäischen und nationalen Nor-
men und technischen Vorschriften, in der zum Unterschrifts-
datum gültigen Fassung, übereinstimmt:

Also conforms with the following European and Na-
tional Standards and technical provisions in the ver-
sion, valid at signature date:

- Technische Regeln für Gefahrstoffe (TRGS) 727:2016,
Vermeidung von Zündgefahren infolge elektrostatischer
Aufladungen

- Technical rules for hazardous substances
TRGS 727:2016, Avoidance of ignition hazards as
consequence of electrostatic charging

Ausgefertigt in Hofheim am 21. März 2019

done at Hofheim on March, 21 2019

Name des Unterzeichners

Name of signatory

Manfred Wenzel

Prokrist / authorized signatory

Unterzeichnet für und im Namen der / Signed for and on behalf of KOBOLD Messring GmbH

Unterschrift / signatur

KEEX68180503

16. Statement of conformity reed contact 41R57**



(1) **Konformitätsaussage** *Statement of Conformity*

(2) - Richtlinie 2014/34/EU - *- Directive 2014/34/EU -*
 Geräte zur bestimmungsgemäßen Verwen- *Equipment Intended for Use in*
 dung in explosionsgefährdeten Bereichen *Potentially Explosive Atmospheres*

(3) Nummer: **ExGuide 18 ATEX 0007**
Document-ID:

(4) Geräte: **Reed-Schalter / Reed contact 41R57 * ***
Equipment:

(5) Hersteller: **KOBOLD Messring GmbH**
Manufacturer:

(6) Anschrift: **Nordring 22-24, DE 65719 Hofheim**
Address:

(7) Die Bauart dieses Produktes, sowie die verschiede- *This product and any acceptable variation thereto is*
 nen zulässigen Ausführungen, sind in der Anlage zu *specified in the enclosure to this Statement of Con-*
 dieser Konformitätsaussage festgelegt. *formity.*

(8) ExGuide Technology - Günter Kämper VDI beschei- *ExGuide Technology - Gunter Kamper VDI certifies*
 nigt, dass dieses Produkt die grundlegenden Sicher- *that this product has been found to comply with the*
 heits- und Gesundheitsanforderungen für die Kon- *Essential Safety and Health Requirements relating*
 zeption von Produkten der Kategorie 3 zur bestim- *to the design and construction of product of Cate-*
 mungsgemäßen Verwendung in explosionsgefährde- *gory 3 intended for use in potentially explosive at-*
 ten Bereichen gemäß Anhang II der Richtlinie erfüllt. *mospheres given in Annex II of the Directive.*
 Das ISO 9001 - System des Unternehmens ExGuide *The ISO 9001 system of ExGuide Technology -*
 Technology - Günter Kämper VDI wird von der GZQ *Gunter Kamper VDI is supervised by GZQ under the*
 unter der Registrierung Q7180217 überwacht. Die *registration number Q7180217.*
 Ergebnisse der sicherheitlichen Betrachtung sind im *The examination and test results are recorded in*
 vertraulichen Dokument D068180222 hinterlegt. *the confidential report number D068180222.*

Seite / page 1 von / of 4 zu / to ExGuide18 ATEX 0007

Diese Konformitätsaussage mit ihren Anhängen darf nur unverändert weiterverbreitet werden.
This statement of conformity and its enclosures may only be reproduced in its entirety and without change.
 ExGuide Technology - Günter Kämper VDI, Birkenstraße 10, DE 44579 Castrop-Rauxel





- (9) Die Erfüllung der grundlegenden Sicherheits- und Gesundheitsanforderungen wird durch Übereinstimmung mit den folgenden Normen bestätigt:
- IEC 60079-0:2017
 - EN 60079-11:2012
- (10) Falls das Zeichen "X" hinter der Nummer (3) steht, wird in der Anlage zur dieser Konformitätsaussage auf besondere Bedingungen für die sichere Anwendung des Produktes hingewiesen.
- (11) Diese Konformitätsaussage bezieht sich nur auf die Konzeption und den Bau des festgelegten Produktes. Weitere Anforderungen dieser Richtlinie gelten für die Herstellung und das Inverkehrbringen.
- (12) Die Kennzeichnung des Produktes soll die folgenden Angaben enthalten:
- Compliance with the Essential Safety and Health Requirements has been assured by compliance with the following standards:*
- If the sign "X" is placed after the Document-ID (3), it indicates that the product is subject to special conditions for safe use specified in the enclosure of this Statement of Conformity.*
- This Statement of Conformity relates only to the design and construction of the specified product. If applicable, further requirements of this Directive apply to the manufacturing and supply of this product.*
- The marking of the product shall include the following:*

 II 3G Ex ic IIC T4 Gc und/oder / and/or
 II 3D Ex ic IIIC T125 °C Dc

$-20\text{ °C} \leq T_a \leq 80\text{ °C}$

ExGuide Technology - Günter Kämper VDI
 Ing.-Büro für Explosionsschutz
 Birkenstraße 10
 DE 44579 Castrop-Rauxel

Telefon: +49 2305 357130
 Telefax: +49 2305 357137

E-Mail: info@exguide.de
 URL: www.exguide.de

Castrop-Rauxel, den 23. Juli 2018

KA68170710 41R57 18 ATEX 0007.odt



Günter Kämper, Inhaber / Owner
 Verbindlich ist die deutsche Fassung / Only the German version is binding

Anlagen / Enclosure

Diese Konformitätsaussage ist ohne Unterschrift ungültig! Im Original sind Teile in roter Schrift dargestellt (Zeile 1, 3, 14 und Logo).

This statement of conformity is not valid without signature! In the original, parts are printed in red (line 1, 3, 14 and logo).

Seite / page 2 von / of 4 zu / to ExGuide 18 ATEX 0007

Diese Konformitätsaussage mit ihren Anhängen darf nur unverändert weiterverbreitet werden.
 This statement of conformity and its enclosures may only be reproduced in its entirety and without change.
 ExGuide Technology - Günter Kämper VDI, Birkenstraße 10, DE 44579 Castrop-Rauxel





(13) Anlage zur

Enclosure to

(14)

Konformitätsaussage

Statement of Conformity

ExGuide 18 ATEX 0007

(15) Beschreibung des Produktes

Description of product

(15a) Die Reed-Schalter arbeiten mit verschiedenen Produkten zusammen und dienen dort zur Signalgabe. Sie sind als Öffner / Schließer oder Wechsler erhältlich.

The reed contact work with different devices and serve signals. They are available as N/C / N/O or change over contacts.

Der elektrische Anschluss erfolgt über einen Stecker – ausschließlich in eigensicheren Anlagen.

The standard electrical connection is made by plugs and sockets – only for intrinsic safety circuits.

(15b) Das Produkt kann folgendermaßen eingesetzt werden:

The product can be used as follows:

a) In der Zone 2 (Gas-Ex, Kategorie 3G, EPL Gc) in den Explosionsgruppen IIA, IIB und IIC

a) In Zone 2 (Gas, Category 3G, EPL Gc) in the explosion groups IIA, IIB and IIC

b) In der Zone 22 (Staub-Ex, Kategorie 3D, EPL Dc) in den Explosionsgruppen IIIA, IIIB und IIIC

b) In Zone 22 (dust hazard, category 3D, EPL Dc) in the explosion groups IIIA, IIIB und IIIC

Die Qualifizierung hinsichtlich der Oberflächentemperatur ist T4; für alle Gase, Dämpfe und Nebel mit einer Zündtemperatur > 135 °C sind die Produkte keine Zündquelle.

The qualification with regard to the surface temperature is T4; for all gases, vapours and mists with an ignition temperature > 135 °C the product is not an ignition source.

Im Staub-Ex-Bereich ist 125 °C die Bezugstemperatur für die weiteren Überlegungen in Hinsicht Sicherheitsabstand von der Glühmtemperatur.

In Dust-Ex-area 125 °C is the reference temperature for further considerations in regard to a safe distance from the smouldering temperature.

Die Anforderungen an einfache elektrische Betriebsmittel in eigensicheren Stromkreisen in der Zone 1 / 21 nach EN 60079-11 werden erfüllt.

The requirements for simple electrical apparatus according to IEC 60079-11, valid for the hazardous area of Zone 1 / 21 are met.

(15c) Elektrische Daten:

Electrical data:

Bemessungsspannung bis 45 Volt AC/DC

rated voltage up to

Bemessungsstrom bis 2 A

rated current up to

$U_{iIC} \leq 30 \text{ V AC/DC}$, $I_{iIC} \leq 250 \text{ mA}$

$U_{iIB} \leq 45 \text{ V AC/DC}$, $I_{iIB} \leq 2 \text{ A}$

$U_{iIIC} \leq 45 \text{ V AC/DC}$, $I_{iIIC} \leq 250 \text{ mA}$

L_i = vernachlässigbar, C_i = vernachlässigbar

L_i = negligible; C_i = negligible

Erwärmung am Außengehäuse < 15 K

warming at the outer enclosure

(15c) Typenschlüssel

Type code

Type No. Description

41R57 A B Type coding

41R57 Contact device

A 3 N/O contact (2 wires), Plug with black cap

6 Change-over contact (3 wires), Plug with grey cap

B * Marking for sensitivity (not ex-relevant)

(15d) Mindestkennzeichnung

Minimum identification of the electrical system:

Hersteller mit Anschrift

Name and address of manufacturer

Typ: 41R57**

Type: 41R57**

(Seriennummer) C € [Baujahr]

(serial number) C € [year of construction]

TFR: 18 ATEX 0007

Ex II 3G Ex ic IIC T4 Gc

Ex II 3D Ex ic IIIC T125 °C Dc

-20 °C ≤ Ta ≤ 80 °C

Seite / page 3 von / of 4 zu / to ExGuide 18 ATEX 0007

Diese Konformitätsaussage mit ihren Anhängen darf nur unverändert weiterverbreitet werden

This statement of conformity and its enclosures may only be reproduced in its entirety and without change.

ExGuide Technology - Günter Kämper VDI, Birkenstraße 10, DE 44579 Castrop-Rauxel





- (Ergänzungen sind zulässig.)
(15e) Die Prüfungsunterlagen sind im internen Dokument D068180222 hinterlegt.
Gemeinsam mit dem Hersteller ist ein vertraulicher Prüfbericht PB68180222 erarbeitet worden.
- (16) Sicherheitstechnische Hinweise
- a) Die Hinweise in der vom Hersteller jedem Produkt beizufügenden Betriebsanleitung (Einbauvorschrift, Montageanweisung) sind unbedingt einzuhalten.
 - b) Zur Sicherstellung des Explosionsschutzes müssen elektrische Betriebsmittel und zusätzlich angebaute (mechanische) Produkte den Anforderungen der vor Ort geltenden Zonen entsprechen und sind vom Errichter der Maschine gesondert zu prüfen.
 - c) An den Stromkreisen dürfen nur Produkte angeschlossen werden, die für den Betrieb in der infrage kommenden Zone geeignet sind und für die die entsprechenden Dokumente vorliegen.
 - d) Der Reed-Schalter ist so zu montieren, dass mögliche elektrostatische Ladungen abfließen können.
 - e) Eine direkte elektrostatische Entladung hoher Energie auf das Betriebsmittel ist nicht zulässig (kann üblicherweise durch eine menschliche Berührung nicht erzeugt werden).
 - f) Der Reed-Schalter sollte gegen mechanische Schlägeinwirkung geschützt eingebaut werden.
 - g) Im Verlauf des eigensicheren Stromkreises ist ein Potentialausgleich zu errichten – wenn der Reed-Schalter über einen geerdeten Stromkreis versorgt wird.
 - h) Festsitzende Teile, z.B. durch Frost oder Korrosion, dürfen bei vorhandener explosionsfähiger Atmosphäre nicht mit Gewalt gelöst werden.
 - i) Die Zündgrenzkurven aus der EN 60079-11 sind in der Zone 2/22 ohne Sicherheitsfaktor zu berücksichtigen und bei der Installation zu beachten.
 - j) In der Zone 1/21 ist der Sicherheitsfaktor 1,5 anzuwenden.
 - k) In jedem Fall hat der Hersteller dazu eine Control Drawing (Nachweis der Eigensicherheit) anzufertigen und der Lieferdokumentation beizufügen.
 - l) Eisbildung am Produkt sollte vermieden werden.
- (17) Besondere Bedingungen
keine
- (Additional hints are allowed.)
Test reports are stored in the internal document D068180222.
Together with the manufacturer a confidential test report PB68180222 has been issued.
Safety relevant notes:
- a) The notes in the operator's manual, enclosed to each order of the manufacturer (installation rules and instructions on assembly), have to be followed strictly.
 - b) In order to ensure the explosion protection required, any electrical and additional mechanical product has to meet the requirements of the locally valid zones and has to be checked separately by the company installing the unit.
 - c) Only products suitable for operation in the relevant zone and for which the relevant documents are available may be connected to the circuits.
 - d) The reed contact has to be mounted in such a manner that any possible electrostatic charges may be discharged.
 - e) Any direct electrostatic discharge of high energy on the product is not permitted (and can usually not be caused by a human touch).
 - f) The installation of the reed contact has to protect them against mechanical impact.
 - g) An equipotential bonding must be installed along of the intrinsically safe circuit - if the reed switch is supplied via an earthed circuit.
 - h) Parts being stuck (e.g. by frost or corrosion) may not be removed by force in the presence of explosive atmosphere.
 - i) In Zone 2/22 the ignition curves of EN 60079-11 have to be observed without safety factor and to be taken into account for the installation.
 - j) The safety factor 1,5 shall be applied in zone 1/21.
 - k) In each case the manufacturer has to create a control drawing (proof of intrinsic safety) to be supplied with the delivery documentation.
 - l) Ice formation on the device must be avoided.
- Special conditions for safe use
none

Seite / page 4 von / of 4 zu / to ExGuide 18 ATEX 0007

Diese Konformitätsaussage mit ihren Anhängen darf nur unverändert weiterverbreitet werden.
This statement of conformity and its enclosures may only be reproduced in its entirety and without change.
ExGuide Technology - Günter Kämper VDI, Birkenstraße 10, DE 44579 Castrop-Rauxel

