

This is your Dry Bath System user manual.

USER MANUAL • BEDIENUNGSANLEITUNG
MODE D'EMPLOI ISTRUZIONI PER L'USO • INSTRUCCIONES DE MANEJO



Passionate for science.



EC Declaration of Conformity

EG-Konformitätserklärung

Wir / We / Nous:

Starlab International GmbH

erklären in alleiniger Verantwortung, dass folgendes Produkt / declare under our sole responsibility that the following product / déclarons sous notre propre responsabilité que le produit ci-dessous

Starlab Dry Bath System, Single Block, Digital. N2400-4001

Starlab Dry Bath System, Dual Block, Digital. N2400-4002

auf das sich diese Erklärung bezieht, mit den folgenden Normen oder normativen Dokumenten übereinstimmt: / to which this declaration relates, is in conformity with the following standards or other normative documents: / auquel se réfère cette déclaration est conforme aux normes ou autres documents normatifs:

EN 61326-1/2006

EN 61326-2-2/2006

Emission: **CISPR 11:2003+A1:2004+A2:2006**
EN 61000-3-2/2006, EN 61000-3-3:2008

Immunity: **IEC 6100-4-2:2008 IEC 61000-4-3:2008**
IEC 6100-4-4:2004+Corr.1:2006+Corr.2:2007,
IEC 61000-4-5:2005
IEC 6100-4-6: 2008, IEC 61000-4-11:2004

Safety: **EN 61010-1: 2001(2nd Edition)**
EN 61010-2-010:2002

Following the Provisions of Directives 2006/95/EC (Low Voltage) and 2004/108/EC (EMC).

Hamburg, 15. Oktober 2020 / October 15, 2020

Certified by:



Klaus Ambos
CEO Starlab International GmbH

Starlab International GmbH
Neuer Höltingbaum 38
22143 Hamburg, Germany
E-Mail: info@starlab.de
www.starlabgroup.com
Tel.: +49 (0)40 675 99 39 0
Fax: +49 (0)40 675 9939 20

Authorised Managing Director
Klaus Ambos

Registry Court
Amtsgericht [first instance court]
Hamburg
Register number: HRB 122020
VAT ID no. pursuant to
§ 27 a German
VAT Act DE 214 891 717

N2400-4001
Dry Bath Heating System, Single Block, Digital

N2400-4002
Dry Bath Heating System, Dual Block, Digital

Table of Contents

Warning 4

1. Information 5

2. Specifications 7

3. Product Description 7

4. Product Overview 8

5. Controls and Features 8

6. Installation Instructions 9

7. Instructions 9

8. Temperature Calibration 10

9. Troubleshooting Guide 10

10. Maintenance 11

11. Ordering information 11

12. Warranty 11



WARNING!

This equipment has been tested and found to comply with the limits for the CE regulation. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy, and if not installed and used in accordance with the instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at their expense. Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment. It is strongly recommended that the user reads the following points before this equipment is operated.

1. Please read and follow the instructions in this manual.

2. Do not alter the equipment. Failure to adhere to these directions could result in personal and / or laboratory hazards, and invalidate the warranty.
3. Use a properly grounded electrical outlet of correct voltage and current handling capacity.
4. Disconnect from the power supply before maintenance and servicing. Servicing should only be carried out by qualified personnel.
5. In the event that solution is accidentally spilled into the instrument, disconnect from the power supply. You must then carry out appropriate decontamination, for eg. turning the unit upside down to avoid the solution contacting the internal components. Remove bottom cover and inspect to assure solution has not contacted elements, thermostat or connector. Any damaged parts will need replacing.
6. Do not use in the presence of flammable or combustible material; fire or explosion may result. This device contains components, which may ignite such materials.
7. Ensure that the system is connected to electrical service according to local and national electrical codes. Failure to properly connect may create a fire or shock hazard.
8. Ensure the appropriate used materials and correct operation to avoid possible hazards of explosion, implosion or release of toxic or flammable gases arising from the materials being heated.
9. Always use the supplied handle to remove hot blocks, and wear appropriate protection to avoid burning your hand.



ATTENTION: Hot surface!

1. Safety Information

As with any electrical device, safety precautions need to be taken. Before connecting with the electrical supply, check the voltage is within the range stated at the rating label and that the device is earthed. Place the unit in a safe and dry location. The unit **MUST NOT** touch anything in the surrounding area. Always follow the safety precautions for chemicals/ dangerous materials, and Hot Surface.

Environmental Conditions

Ensure the instrument is installed and operated strictly in the following conditions:
< = 95 % RH, 75 KPa-106 Kpa. Altitude must not exceed 2000 meters.

Avoiding Electrical Shock

Please follow the guidelines below to ensure safe operation of the unit. The Starlab Dry Bath Heating System has been designed for use with shielded wires, thus minimising any potential shock hazard to the user. Starlab does not recommend the use of unshielded wires.

1. NEVER connect/disconnect wire leads from the power jacks when the red indicator light on the START button is on, or when "RUNNING" is displayed on the LCD screen.
2. WAIT at least 5 seconds after stopping a run before handling output leads or connected apparatus.
3. ALWAYS make sure that your hands or gloves, the work area and any instruments used, are clean and dry before making any connections or operating the power supply.
4. ONLY connect the power cord to a properly grounded AC outlet.

Avoiding Damage to the Instrument

1. Do not attempt to operate if the unit is damaged in any way.
2. Protect the unit from physical damage, corrosive agents, and extreme temperatures (direct sunlight etc).
3. For proper ventilation, the unit should be situated and operated with at least 10 cm of clear space behind and at least 5 cm of clear space on either side.
4. Do not operate the Starlab Dry Bath Heating System in high humidity environments (> 95 %), or where condensation may occur.
5. Before using any cleaning or decontamination method (except those recommended in this manual), you should check with Starlab or your Starlab distributor that the proposed method will not damage the equipment.



Equipment Operation

Follow the guidelines below to ensure safe operation of the unit:
Features

1. To avoid significant discrepancies between set temperature and temperature reached, please monitor the displayed temperature regularly eg. by using a calibrated laboratory thermometer. See page 9 “Temperature Calibration” for detailed information.
2. NEVER access any HAZARDOUS LIVE parts.
3. Do not apply lids or covers to any of the tubes being heated in the Starlab Dry Bath Heating System in order to prevent the possible hazard of explosion and consequent damage.

Symbols

The symbols used on the Starlab Dry Bath Heating System are explained below.



Danger Electricity: indicates a potential shock hazard may exist.



General Warning: indicates possible personal injury or instrument damage.



ATTENTION: Hot surface!

2. Specifications

Controller	Digital Microprocessor Controller
Display	Digital
Operating Temperature	5 °C above ambient, to 150 °C
Temperature Increase	0.1 °C
Temperature Calibration	Yes
Temperature Uniformity	± 0.2 °C at 37 °C
Temperature Accuracy	± 0.2 °C at 37 °C
Timer	0 to 999 minutes
Safety Device	Leak-proof heating chamber
Heating Chamber Material	PTFE-coated aluminium
Block Material	Aluminium
Block Dimensions	79 x 104 x 50mm (except N2400-4108)
Water Bath Volume (approx.)	Single: 400 ml. Dual: 800 ml
Data Log	RS 232 (Maximum 2.5 m long)
Power	N2400-4001: 125 W; N2400-4002: 200 W
Rated Voltages	110 or 220 Volts. N2400-4001: 220 V AC, 50/60 Hz, 0.63 A. N2400-4002: 220 V AC, 50/60 Hz, 1 A.
Unit Dimensions	200 x 298 x 80 mm (w x l x h)
Weight	N2400-4001: 2.1 kg; N2400-4002: 2.8 kg

3. Product Description

The single block (N2400-4001) and dual block (N2400-4002) units use interchangeable heating block modules for a variety of applications, including restriction digests, denaturing DNA, BUN, melting agar, coagulation studies, in-situ hybridization and Hot Start thermo-cycler reaction, as well as having the additional function of being used as a water bath. All models incorporate a PID controller for easy temperature selection, rapid heat-up, and excellent stability. Temperature may be set in 0.1 °C increments, from 5 °C above ambient to 150 °C. The timer can be set from 0 to 999 minutes for the user's convenience.

Features



- Digital performance at analog prices
- Microprocessor controller with digital display
- Easy, user calibration
- Leak-proof aluminium heating chamber
- Single and dual block modes



4. Product Overview

Starlab Dry Bath Heating Systems are designed to cover a wide variety of applications. Excellent temperature control delivers accurate and reliable experimental results, time after time. Starlab Dry Bath Heating Systems are space-saving, compact instruments, offering great value and convenience for the user. All units comply with CE regulations.

5. Controls and Features

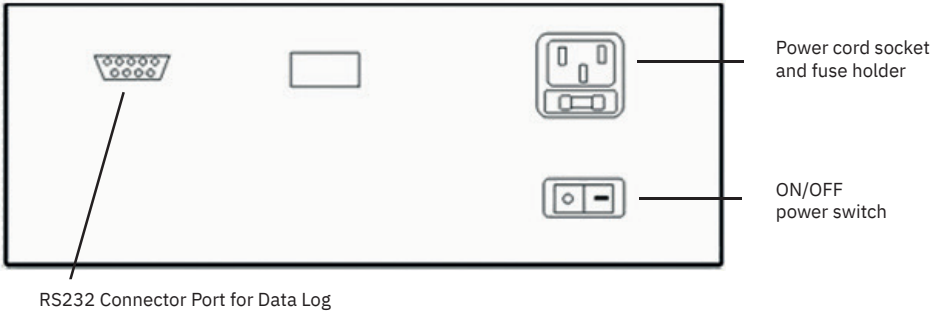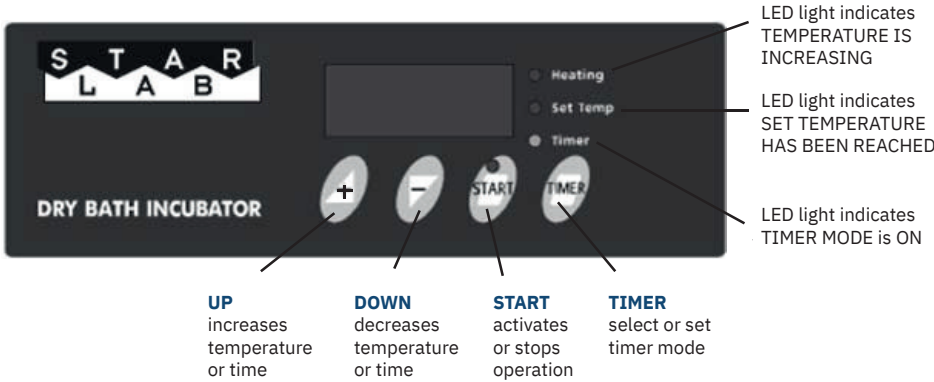

6. Installation Instructions

The Starlab Dry Bath Heating Systems are ready to 'Plug and Play'. The unit should only be used on a sturdy, level surface in a safe, dry place. Before operation, ensure one or two heating aluminium block(s) is / are inserted into the bath, or if using as a water bath, that water has been added.

7. Operating Instructions

1. Place the unit on a sturdy, level surface in a safe, dry place, away from laboratory traffic.
2. Ensure that the AC power switch is OFF, then plug the power cord into a grounded AC outlet of appropriate voltage (115 V or 220 V as indicated on the rating sticker near the AC cord on the back of the unit).
3. Select a suitable metal block(s), or the appropriate water volume if using as a water bath, and put into the unit.
4. Turn the AC power ON.
5. Use the UP or DOWN Key to adjust to the desired temperature.
6. Press the START Key to start heating.
7. To change the temperature during heating, press START again to deactivate and set the new temperature. Press START to activate heating.
8. Press the START key again, to stop the unit.

NOTE: If setting the **heating time** is required, press the TIMER Key, and then press the UP or DOWN Key to adjust the time accordingly. The unit will 'auto-stop' when the time is up.

Protection/Error Messages


Error Types	Description
Err1	If the displayed temperature value is 5 °C over the set temperature value, Err1 will be displayed, an alarm will sound and the instrument will shut down automatically.
Err2	If the displayed temperature value reaches a temperature much higher than the set temperature value within 1 minute of the unit being switched on, Err2 will be displayed and an alarm will sound. This problem is due to SSR.
Err3	If the internal temperature sensor is broken or a connection problem occurs, Err3 will be displayed; an alarm will sound, and the instrument will shut down automatically.



8. Temperature Calibration

The Starlab Dry Heating System with (optional) metal heating blocks has been calibrated as a set. However, the different kinds of block do not generate the same results. Therefore, for optimum temperature control accuracy, and when changing to different kinds of block, the unit should be calibrated using the procedure outlined below.

- 1. Insert a calibrated, 45 mm laboratory thermometer into the Thermometer holding port on the block.
- 2. SIMULTANEOUSLY Press the ON/OFF power switch on the back of the unit and the START Key on the front. During this, the unit will omit a “DU~DU” sound and a LED segment will be flashing (see below). The unit is now in ‘Calibration Mode’.

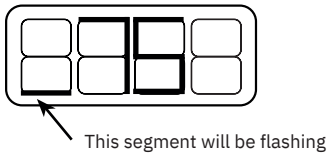

- 3. Press the UP or DOWN key to adjust the value displayed to the required temperature, then press the START key.
- 4. Wait for around 40 to 50 minutes until all the LED segments are flashing.
- 5. Adjust the display value to the same figure as the thermometer, then press the START key.
- 6. The calibration procedure is now finished. Please wait for a few minutes so the microprocessor has time to auto-adjust the temperature, and the LED display value is the same as thermometer.

9. Troubleshooting Guide

Many operating problems may be solved by reading and following the instructions in this manual. Some suggestions for troubleshooting are given below. Should these suggestions not resolve the problem, contact Starlab or your Starlab distributor for assistance.

Problem	Recommendations
LED does not light up	Check the FUSE
	Ensure that the AC power switch is ON
	Check the power cord is properly plugged into a grounded AC outlet of appropriate voltage



10. Maintenance

The Starlab Dry Bath Heating System may be cleaned with a moist cloth containing a mild soap solution. The blocks are aluminum and may be cleaned with any of the commercial aluminum cleaners on the market.

11. Ordering Information

Article No.	Description
N2400-4001	Starlab Dry Bath Heating System, Single Block*, Digital
N2400-4002	Starlab Dry Bath Heating System, Dual Block*, Digital
N2400-4100	Metal Block for 64 x 0.2 ml PCR Tubes
N2400-4101	Metal Block for 20 x 1.5/2.0 ml Microcentrifuge Tubes
N2400-4102	Metal Block for 12 x 15 ml Centrifuge Tubes
N2400-4103	Metal Block for 4 x 50 ml Centrifuge Tubes
N2400-4104	Metal Block for 20 x 1.5/2.0 ml Microcentrifuge Tubes (V-Bottoms)
N2400-4105	Metal Block for 20 x 0.5 ml Tubes
N2400-4106	Metal Block for 20 x 13 mm Diam. Tubes
N2400-4107	Metal Block for 96-Well PCR Plate (for Single Block System)
N2400-4108	Metal Block for 96-Well PCR Plate (for Dual Block System)

* Metal block(s) not included. Metal blocks must be purchased separately.

Further Metal Block configurations or customised blocks may also be available. Contact Starlab for details.

12. Warranty

The Starlab Dry Bath Heating System is under warranty, against defects in materials and workmanship under normal service, for two years from the shipping date to the purchaser. This warranty excludes damages resulting from misuse, carelessness, or neglect. Starlab's liability under the warranty is limited to the receipt of reasonable proof from the customer that the defect is embraced within the terms of the warranty. All claims made under this warranty must be presented to Starlab or a Starlab Distributor within two years following the date of delivery of the product.



**Starlab
International GmbH**

Neuer Hölftigbaum 38
22143 Hamburg
Germany

T: +49 (0)40 675 99 39 0
F: +49 (0)40 675 99 39 20
info@starlab.de
www.starlabgroup.com

Starlab GmbH

Neuer Hölftigbaum 38
22143 Hamburg
Germany

T: +49 (0)40 675 99 39 0
F: +49 (0)40 675 99 39 20
info@starlab.de
www.starlab.de

Starlab (UK), Ltd

5 Tanners Drive
Milton Keynes MK14 5BU
United Kingdom

T: +44 (0)1908 283800
F: +44 (0)1908 283802
info@starlab.co.uk
www.starlab.co.uk

Starlab France SARL

30 Rue Jean Rostand
91400 Orsay
France

T: +33 (0)1 60 1371 70
F: +33 (0)1 69 4148 65
info@starlab.fr
www.starlab.fr

Starlab S.r.l.

Via Pinturicchio 1
20133 Milano
Italy

T: +39 (0)2 7020 1040
F: +39 (0)2 7020 1033
info@starlab.it
www.starlab.it

IMDB-INF-INT-01-2021

Passionate for science.

